


Accellix Beads and Cytokines



Accellix Beads and Cytokines

Sample #	IL-6 Conc. (pg/ml)	Molarity (fM)	Mean Fluorescence Intensity	Normalized Fluorescence Intensity
0	0	0	251	0
1	1.25	50	278	27
2	2.5	100	301	50
3	5	200	332	81
4	10	400	410	159

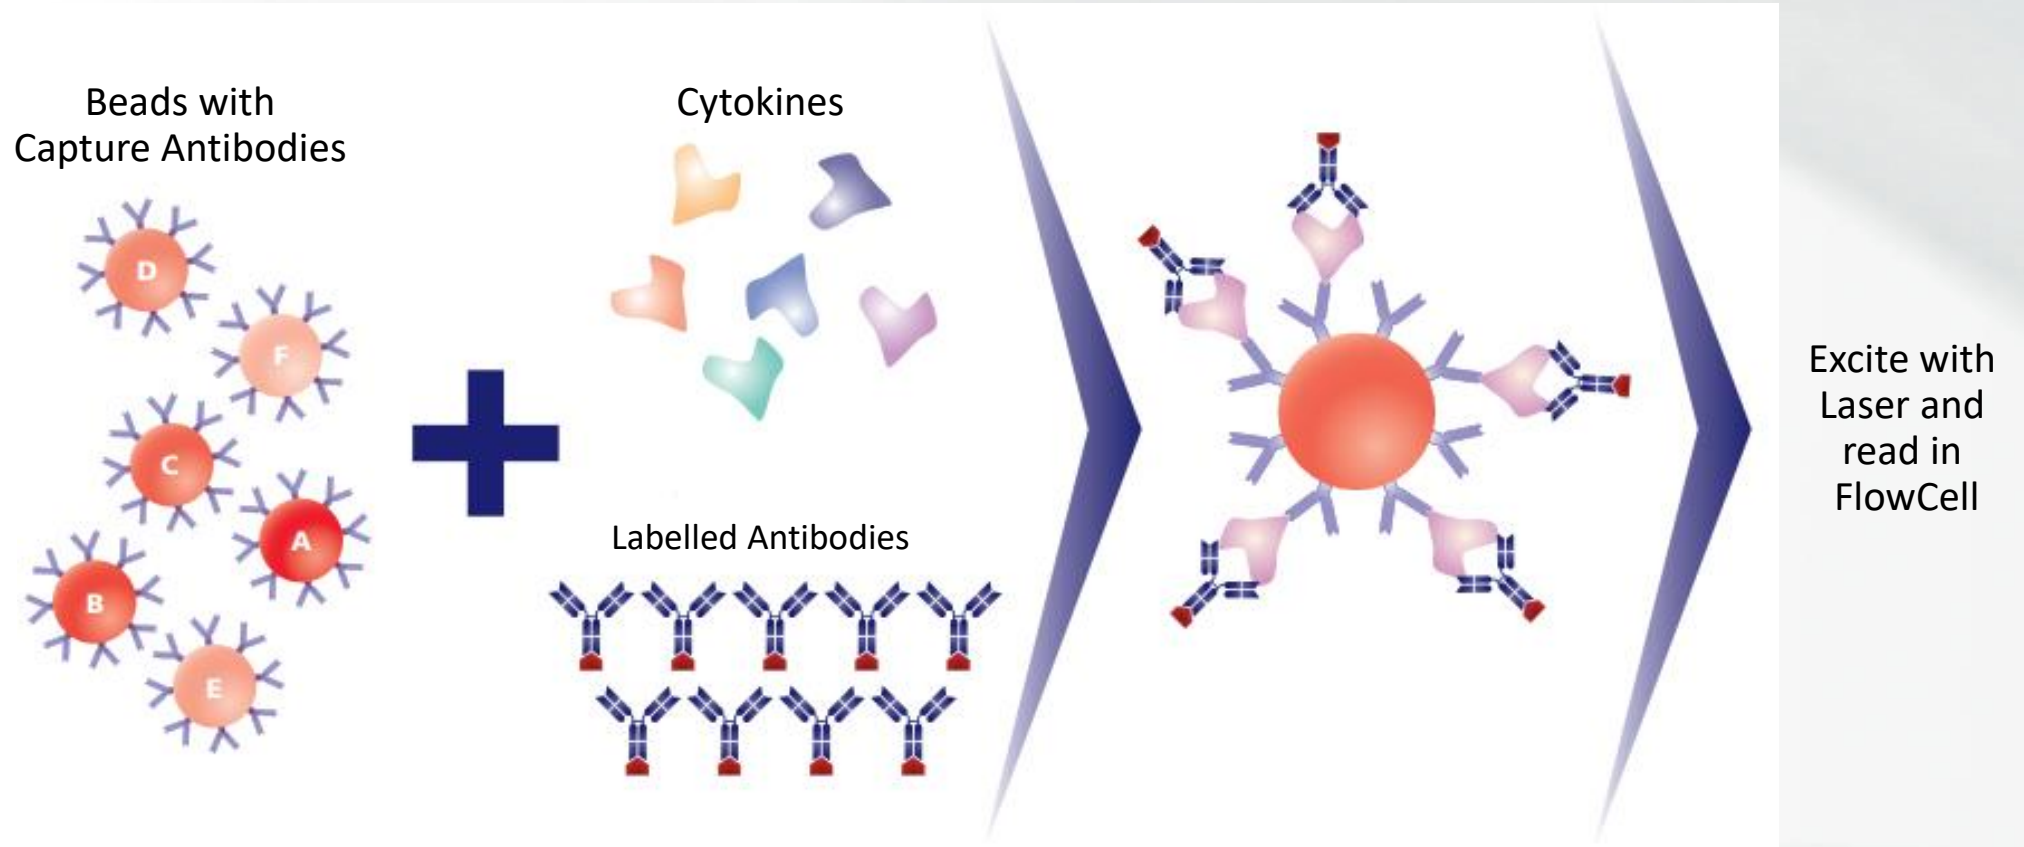